


# Airo<sup>®</sup> TruCT<sup>®</sup>

Service excellence

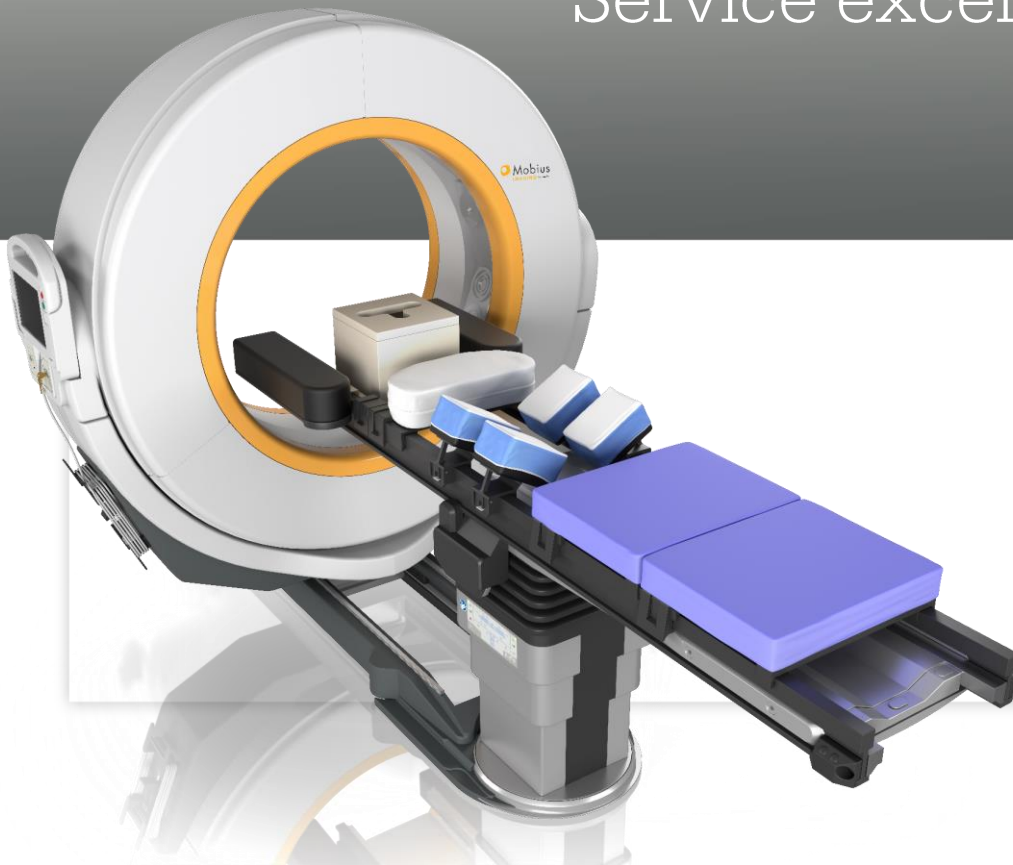

Did you  
**know?**

Our **Enabling Technologies Service Team** is dedicated to **Airo<sup>®</sup>** support and service. Our goal is to ensure your Airo<sup>®</sup> TruCT<sup>®</sup> system is maintained to the highest quality standards and remains functional.

## What can I expect from **Airo** Service Packages?

	<b>Prevent</b>	<b>Protect</b>
<b>Bi-annual preventative maintenance at your facility</b>	✓	✓
Inspection, calibration, tube alignment and replacement of specified parts	✓	✓
Update to the latest AIRO software version; OS bug fixes, patches, etc.	✓	✓
Travel and labor costs for your technician	✓	✓
Detailed service report and any applicable compliance documentation for inspected items*	✓	✓
<b>Unlimited** repairs</b>		✓
All related parts, installation, testing, labor and shipments included		✓
Priority first assessment is done within 24 hours from the service call (one (1) working day)		✓
Discount on all other upgrades (new features) and clinical trainings		✓

\*Refer to the Service Agreement contract for a detailed list of applicable parts \*\*Check Terms and Conditions for applicable repair calls



### **Minimize system downtime**

Dedicated Airo Support Team



### **Airo software upgrades**

First access to upgrades and updates

This document is intended solely for the use of healthcare professionals. A healthcare professional must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that healthcare professionals be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate the breadth of Stryker product offerings. A healthcare professional must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area. Service plans will be subject to the terms and conditions outlined in the service contract. Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Airo, Stryker, TruCT. All other trademarks are trademarks of their respective owners or holders. The medical devices depicted are CE marked in accordance with applicable EU Regulations and Directives. The material is not intended for distribution outside the EU and EFTA.

Stryker European Operations Herikerbergweg 1101101 CM Amsterdam Netherlands P: + 3120219 2600